6044 Cornerstone Court W, Ste E
San Diego, CA 921211
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

Data Sheet

Kinetic HDAC2 Assay Kit

Catalog #: 53002

DESCRIPTION: The *Kinetic HDAC2 Assay Kit* is a complete assay system designed to measure histone deacetylase 2 (HDAC2) activity kinetically for screening and profiling applications. It comes in a convenient 96-well format, with all the reagents necessary for 100 fluorescent HDAC2 activity measurements. In addition, the kit includes purified HDAC2 enzyme and a potent HDAC inhibitor, SAHA, for use as a positive and negative control. The *Kinetic HDAC2 Assay Kit* is based on a unique fluorogenic substrate and developer combination. This assay method eliminates dealing with the radioactivity, extraction, and chromatography aspects of traditional assays. Using this kit, only one simple step for setting up the HDAC2 reaction on a microtiter plate is needed and then the HDAC2 activity level can be measured kinetically using a fluorescence reader.

COMPONENTS:

Catalog #	Reagent	Amount	Storage	
50002	HDAC2 human recombinant enzyme	5 µg	-80°C	***Avoid Freeze/ Thaw Cycles!***
50037	Fluorogenic HDAC substrate 3 (5 mM)	50 µl	-80°C	
53029	10x HDAC Developer	1 ml	-80°C	
	Developer Dilution Buffer	10 ml	-20°C	
	SAHA (1 mM)	20 µl	-20°C	
50031	HDAC Assay Buffer	20 ml	-20°C	
	BSA (1mg/ml)	1 ml	-20°C	
79685	black, low binding NUNC black microtiter plate	1 plate	Room temp.	

MATERIALS OR INSTRUMENTS REQUIRED BUT NOT SUPPLIED:
Fluorescent microplate reader

APPLICATIONS: Great for studying enzyme kinetics and screening small molecular inhibitors for drug discovery and HTS applications.

STABILITY: One year from date of receipt when stored as directed.

REFERENCE(S):

1. Santo, L., *et al., Blood.* 2012 Mar 15;**119(11)**:2579-89.
2. Bradner, J.E., *et al., Nat Chem Biol.* 2010 Mar;**6(3)**: 238-243.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.
To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
Or you can Email us at: **info@bpsbioscience.com**
Please visit our website at: **www.bpsbioscience.com**

6044 Cornerstone Court W, Ste E
San Diego, CA 921211
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

ASSAY PROTOCOL:

Thaw all of the components except the HDAC enzyme, and place on ice. All of the reactions should be set up on ice.

1) Prepare the master **HDAC Substrate Solution**
   To make the master **HDAC Substrate Solution,** mix 2368 µl **HDAC Assay Buffer,** 800 µl BSA (1mg/ml), and 32 µl **HDAC Substrate.** This is enough for 100 reactions. If you have less than 100 reactions, you can reduce the components proportionally. (Make sufficient quantity needed for the assay; store remaining BSA and 5 mM stock solution in aliquots at -80°C.)

   Add 20 µl of the master **HDAC Substrate Solution** to each well.

2) Prepare **Inhibitor Solutions**
   Dilute the Test Inhibitor 10-fold higher than the final concentration you want to test in 10% DMSO (the final DMSO concentration is 1% in all of the reactions).

   Dilute the same buffer without the inhibitor (Inhibitor Buffer) in 10% DMSO as a control.

   Add 10 µl of the **Test Inhibitor Solution** to each well designated as "Test Inhibitor", and 10 µl of **SAHA Solution** to each well designated as "SAHA Inhibitor Control". Add 10 µl of 10% DMSO to each well designated "Blank" and "Positive Control".

3) Prepare **Developer solution**
   Dilute the **10X Developer Solution** (1:10 dilution) in **Developer Dilution Buffer.**

   Add 50 µl of the **Developer Solution** to each well.

4) Prepare **HDAC2 Enzyme Solution**
   Dilute **HDAC2** in HDAC assay buffer to 2 ng/µl (40 ng/reaction). Aliquot any remaining enzyme and store undiluted at -80°C.

   Add 20 µl of HDAC assay buffer to each well designed "Blank". Add 20 µl of the **HDAC1 enzyme solution** to each well designed "Positive Control", "Test Inhibitor" and "SAHA Inhibitor Control". **Always add the enzyme solution last.**

5) Measure the plate in 5 minute intervals for a period of up to one hour, using a microtiter plate-reading fluorimeter capable of excitation in the range of 350-380

6044 Cornerstone Court W, Ste E
San Diego, CA 921211
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

nm and detection of emitted light in the range of 440-460 nm. The "Blank" value is subtracted from all other values.

	"Blank"	Positive Control	Test Inhibitor	SAHA Inhibitor Control
Master HDAC Substrate Solution	20 µl	20 µl	20 µl	20 µl
SAHA	–	–	–	10 µl
Test Inhibitor	–	–	10 µl	–
Inhibitor buffer (no inhibitor)	10 µl	10 µl	–	
1X Developer	50 µl	50 µl	50 µl	50 µl
HDAC assay buffer	20 µl	–	–	–
HDAC2 (2 ng/µl)	–	20 µl	20 µl	20 µl
Total	100 µl	100 µl	100 µl	100 µl

Example of Assay Results:

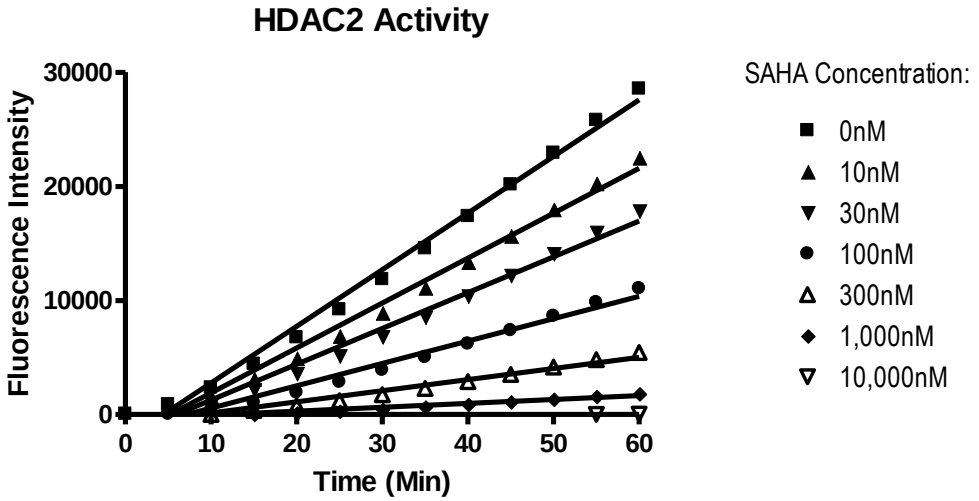

Figure 1. Time course of HDAC2 activity against different concentrations of SAHA, measured using the *Kinetic HDAC2 Assay Kit*, BPS Bioscience Cat# 53002. Fluorescence was measured using a Tecan fluorescent microplate reader. *Data shown is lot-specific. For lot-specific information, please contact BPS Bioscience, Inc. at info@bpsbioscience.com.*

6044 Cornerstone Court W, Ste E
San Diego, CA 921211
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

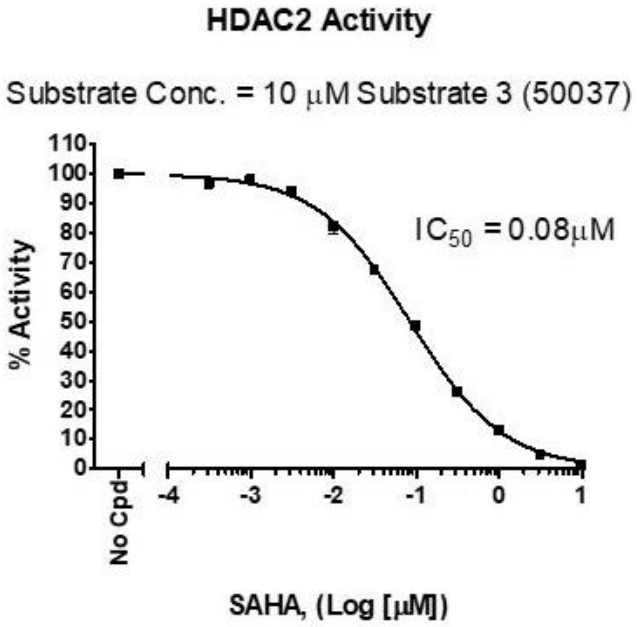

Figure 2. IC50 assay of HDAC2 against SAHA.

6044 Cornerstone Court W, Ste E
San Diego, CA 921211
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

RELATED PRODUCTS:

Product Name	Catalog #	Size
HDAC1	50051	50 µg
HDAC2 (C-Flag)	50052	50 µg
HDAC3/NcoR2	50003	50 µg
HDAC4	50004	10 µg
HDAC5	50005	10 µg
HDAC6 (C-Flag)	50056	50 µg
HDAC7	50007	10 µg
HDAC8	50008	50 µg
HDAC9	50009	10 µg
HDAC10	50010	50 µg
HDAC11	50011	50 µg
HDAC Assay Kit	50033	96 reactions
HDAC Assay Kit (Green)	50034	96 reactions
HDAC Class 2a Assay Kit	50041	96 reactions
HDAC1 Assay Kit	50061	96 reactions
HDAC2 Assay Kit	50062	96 reactions
HDAC3 Assay Kit	50073	96 reactions
HDAC4 Assay Kit	50064	96 reactions
HDAC5 Assay Kit	50065	96 reactions
HDAC6 Assay Kit	50076	96 reactions
HDAC7 Assay Kit	50067	96 reactions
HDAC8 Assay Kit	50068	96 reactions
HDAC9 Assay Kit	50069	96 reactions

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.
To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
Or you can Email us at: **info@bpsbioscience.com**
Please visit our website at: **www.bpsbioscience.com**